

REPLACEMENT SHEET

6/14

/


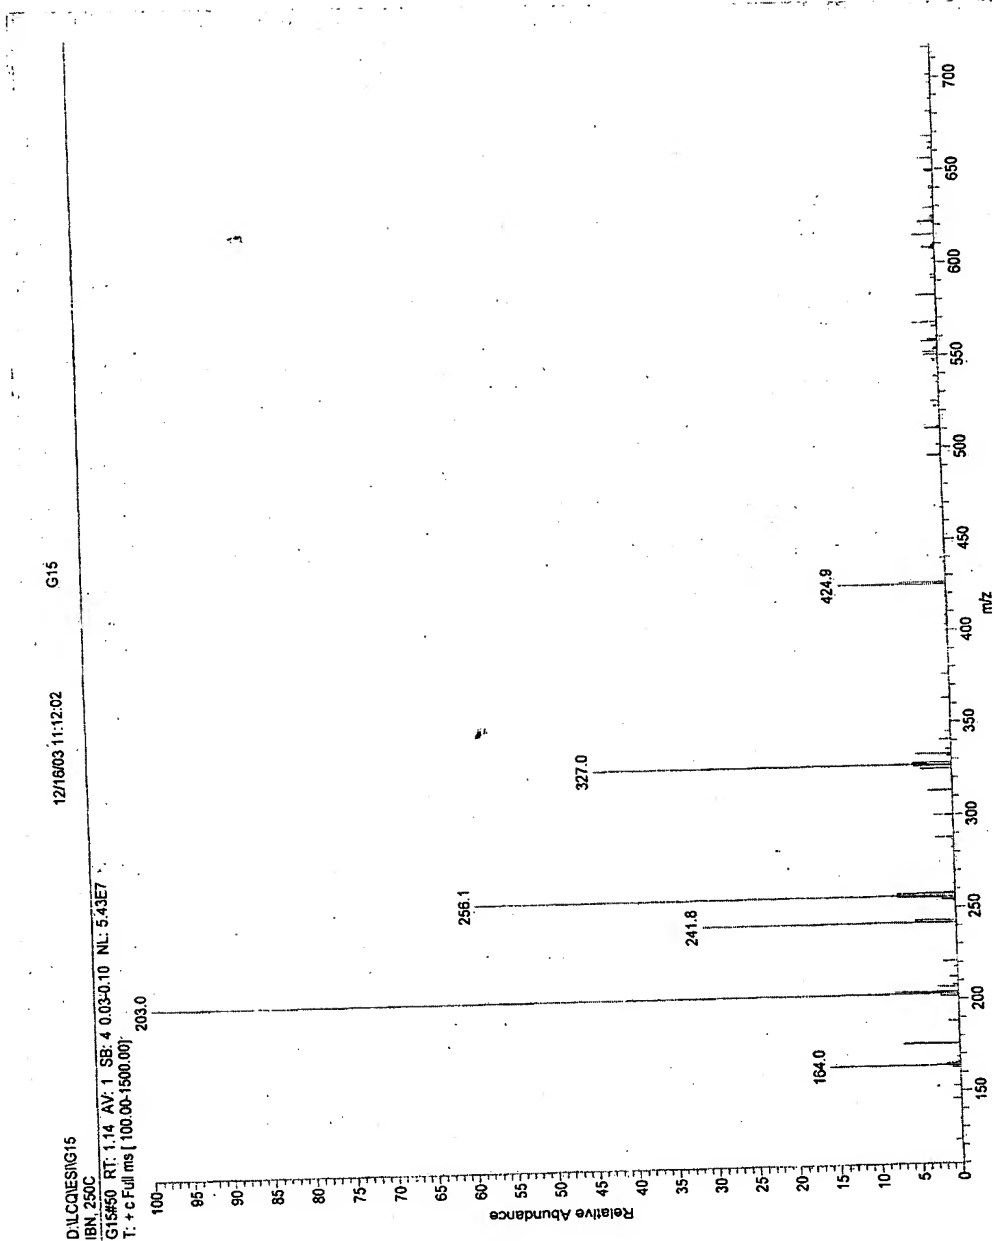


FIGURE 7A

BEST AVAILABLE COPY

7/14

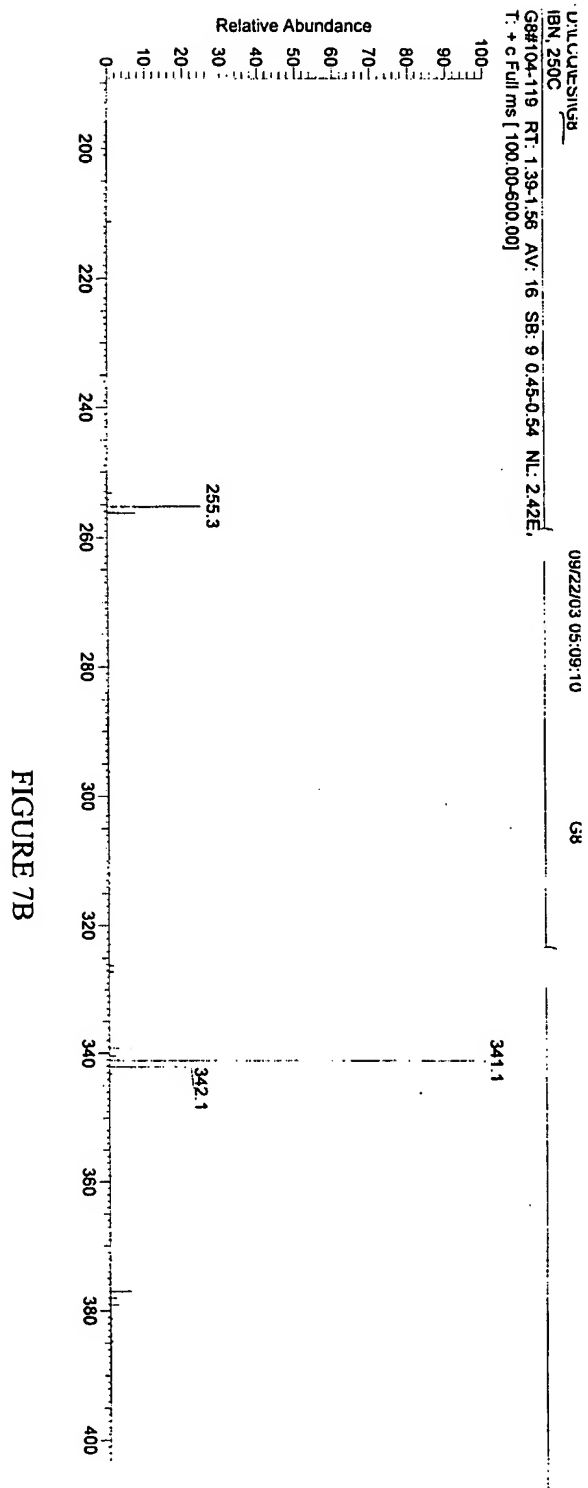

BEST AVAILABLE COPY

10/14

IBN DR GAO ZHIQIANG 1H DPX300
GS (WITH WATER SUPPRESSION)

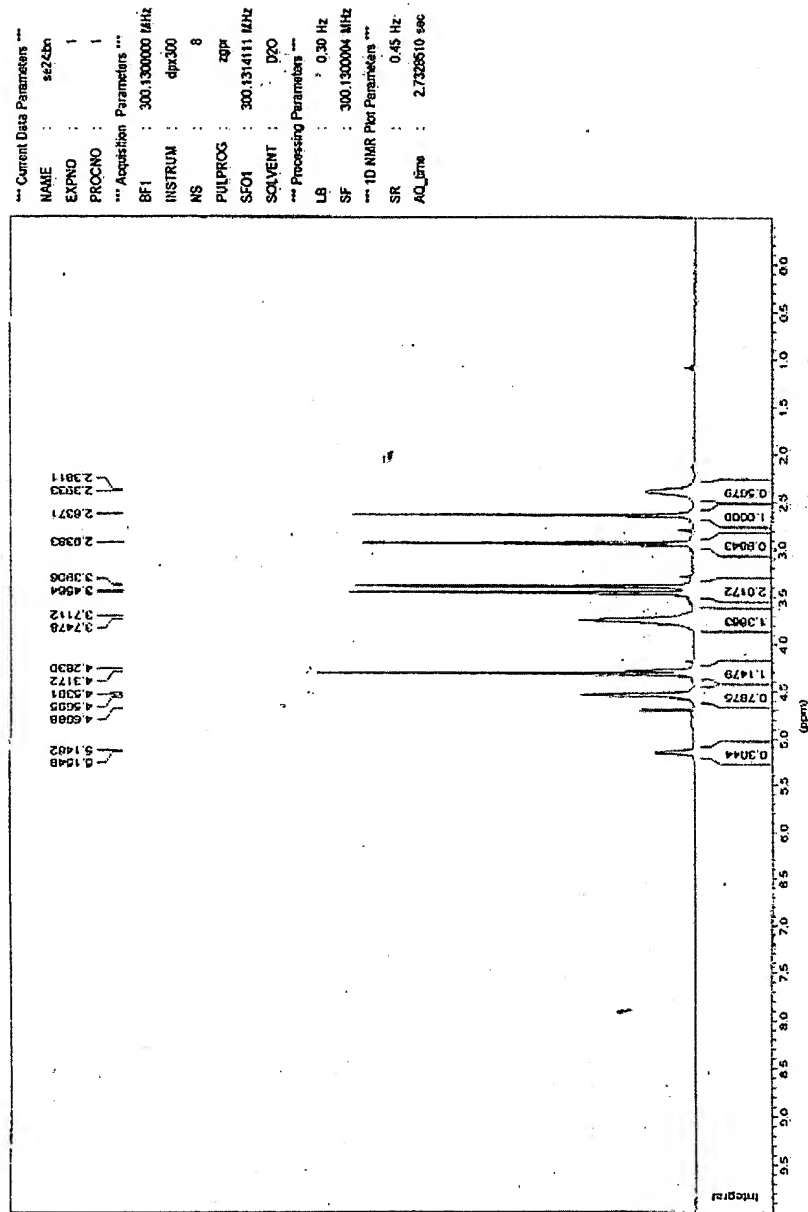


FIGURE 9A

BEST AVAILABLE COPY

11/14

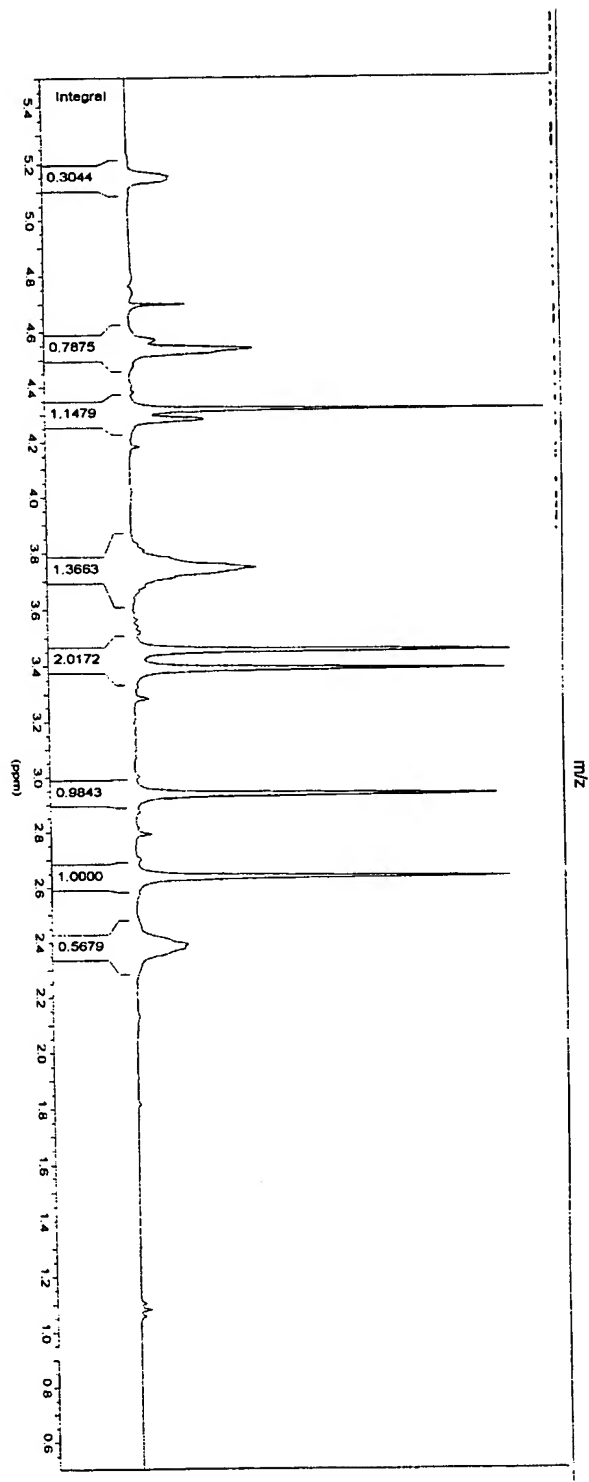


FIGURE 9B

BEST AVAILABLE COPY